


Results according to the stricture etiology

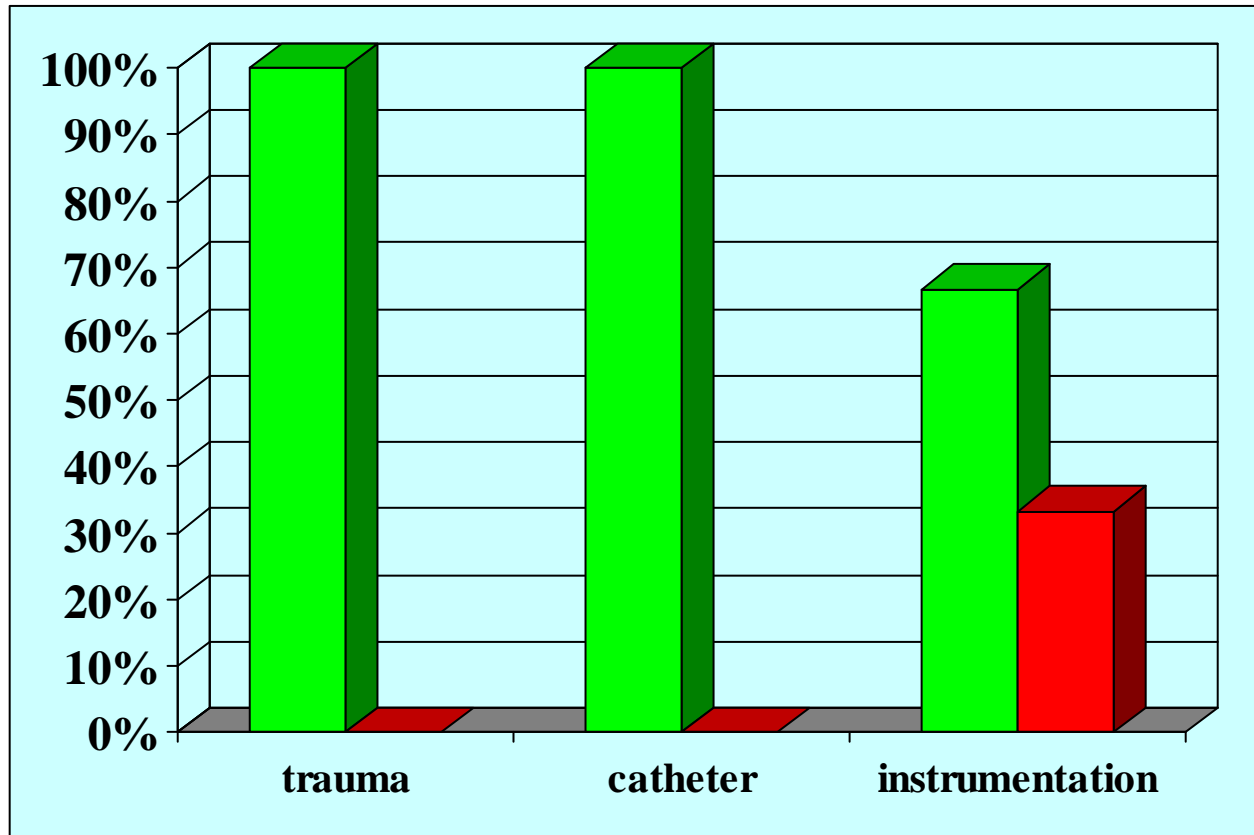

	trauma	catheter	instrumentation
■ success	1 (100%)	1 (100%)	2 (66.7%)
■ failure	/	/	1 (33.3%)