


## Results according to the stricture etiology

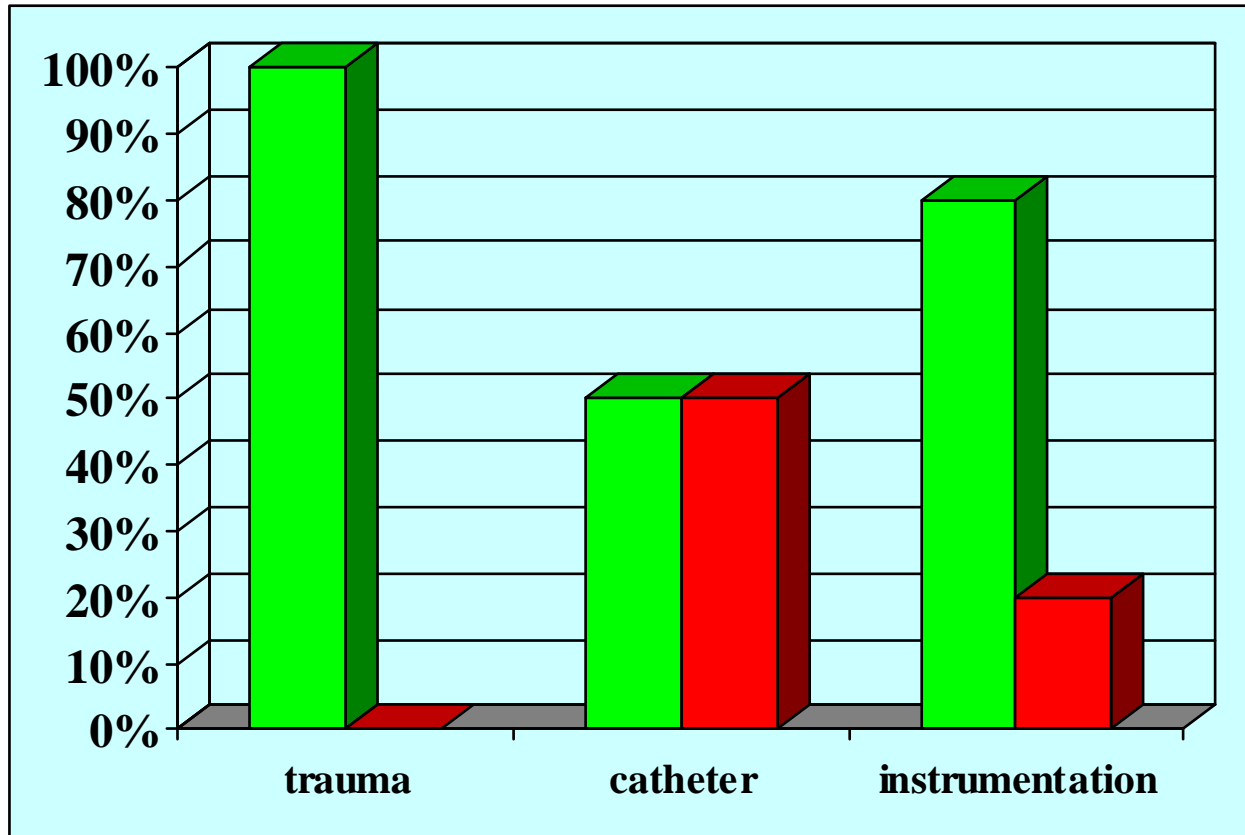

	trauma	catheter	instrumentation
■ success	1 (100%)	1 (50%)	4 (80%)
■ failure	/	1 (50%)	1 (20%)