


Results according to the stricture etiology

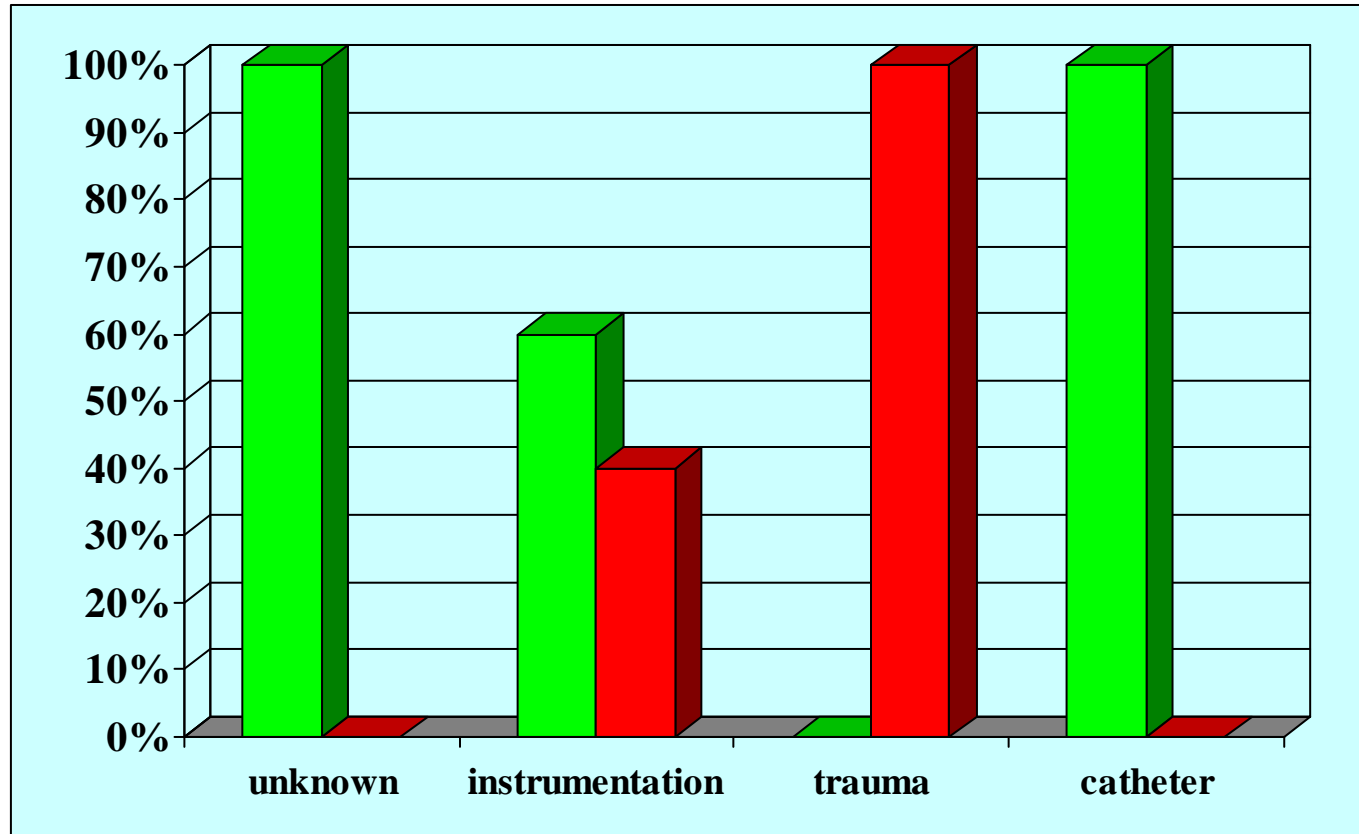

	unknown	instrumentation	trauma	catheter
■ success	4 (100%)	3 (60%)	/	2 (100%)
■ failure	/	2 (40%)	1 (100%)	/