


Results according to the stricture etiology

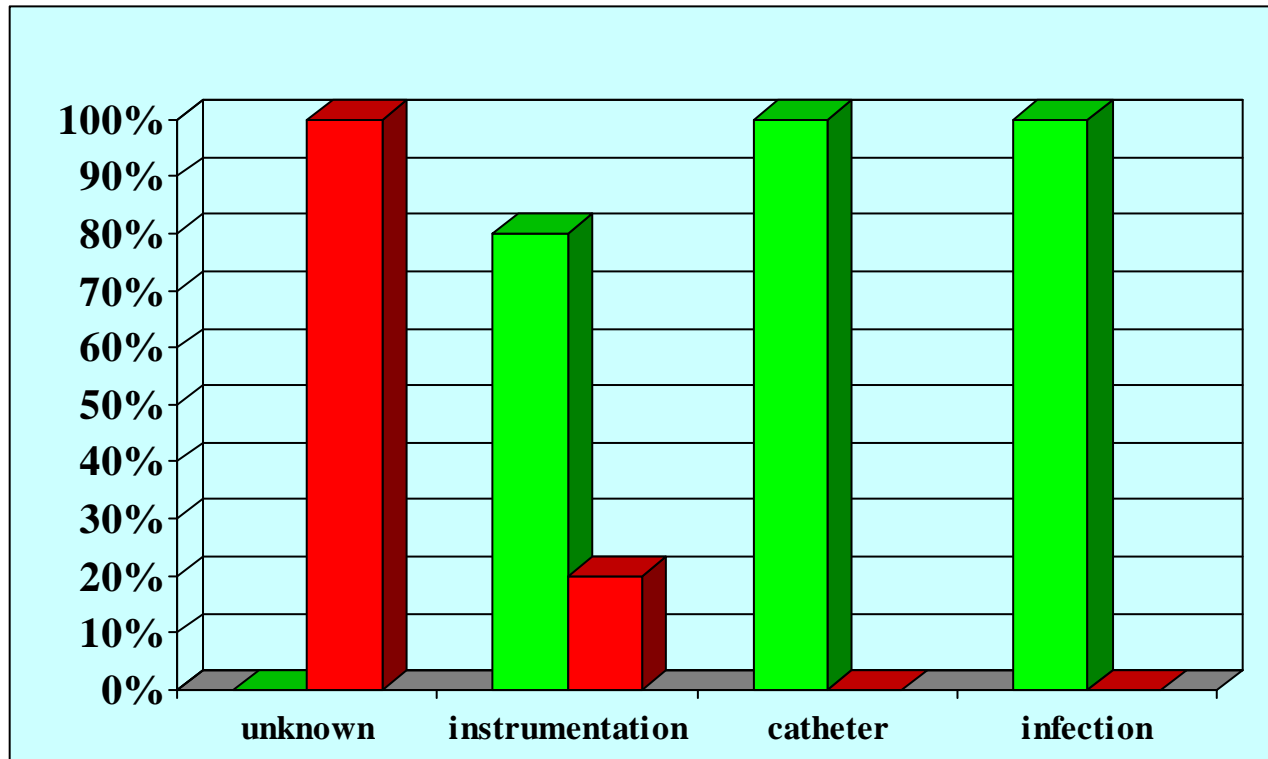

	unknown	instrumentation	catheter	infection
■ success	/	4 (80%)	2 (100%)	1 (100%)
■ failure	4 (100%)	1 (20%)	/	/